



# Reference Guide

*Short-form instruction  
for powering on and using the  
Ventis™ Pro4 Multi-Gas Monitor and the  
Ventis™ Pro5 Multi-Gas Monitor*

Edition: 3  
March 23, 2016  
Part Number: 17156495-1

**INDUSTRIAL**  

---

**SCIENTIFIC**

Industrial Scientific Corporation, Pittsburgh, PA USA

Industrial Scientific Co., Ltd. Shanghai, China

© 2016 Industrial Scientific Corporation

All rights reserved. Published 2016.

Revision 3



# Contents

Attention Safety Team .....	1
Hardware Overview .....	2
Pump Installation and Preparation .....	4
Power On .....	6
User-site Assignments .....	9
Instrument Operation .....	10
Alarms, Warnings, and Indicators .....	13
Power Off .....	17

## List of abbreviations

DSSAC	Docking Station Software Admin Console
ppm	parts per million
TWA	time-weighted average
STEL	short-term exposure limit

Thank you for choosing the Ventis™ Pro Series from Industrial Scientific Corporation!

## Attention Safety Team

Reference Guide content is limited to abbreviated instruction for powering on and using the Ventis™ Pro4 Multi-Gas Monitor and Ventis™ Pro5 Multi-Gas Monitor. Derived from parts of the *Product Manual*\*, it is not a substitute for the manual. Use this guide, the product manual, and other Industrial Scientific services—in combination with your own resources—to prepare workers for successfully using the instruments in your gas-monitoring environment.

Get off to a good start with your new Ventis Pro Series instrument. Before using it for the first time:

- ✓ Read and understand the *Product Manual*\*.
- ✓ Review the unit's settings and adjust them as needed.
- ✓ Train instrument users.
- ✓ Charge the unit's battery.
- ✓ Calibrate the instrument, then complete a bump test.

\*The *Product Manual* is available online at [www.indsci.com/ventispro](http://www.indsci.com/ventispro).

### Need help?


Contact the gas detection experts at Industrial Scientific!

- Technical Support
- Training
- Ask Dave


[www.indsci.com](http://www.indsci.com)

# Hardware Overview

Ventis Pro Series diffusion instrument (Ventis Pro5 shown)

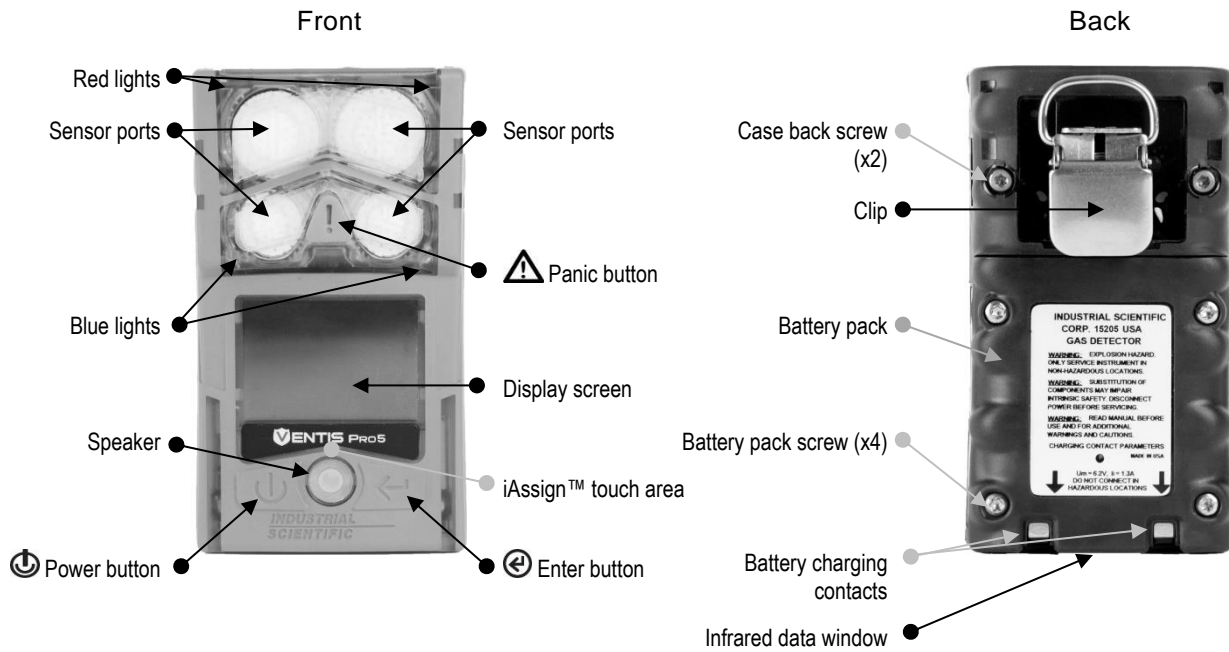

Ventis Pro Series aspirated instrument (Ventis Pro5 shown)

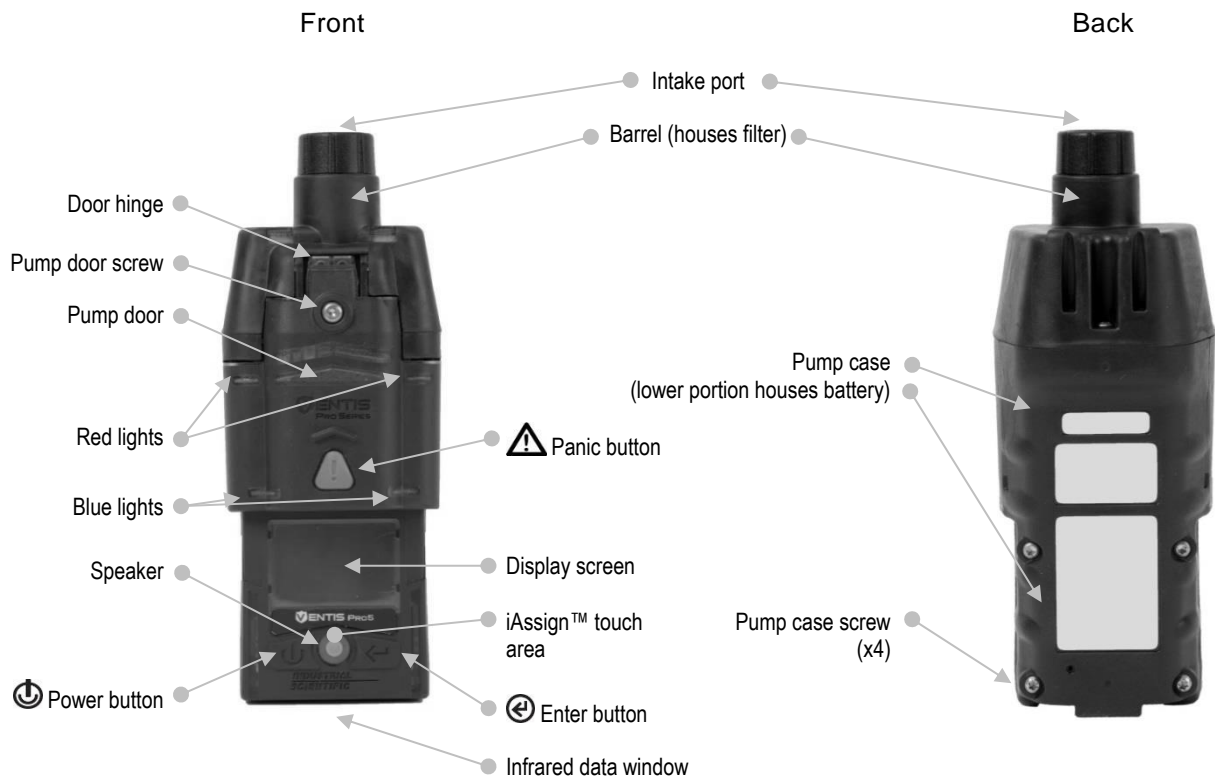

# Pump Installation and Preparation

If the instrument will be used without a pump, skip to page 6.

To use the instrument with its integrated pump, complete one or both instruction sets below.

- If the pump is *not* installed, follow the instructions below for both pump installation and pump preparation.
- If the pump *is* installed, follow the instruction below for pump preparation only.

## Pump installation

---



Unscrew and remove the belt clip. Store the clip, screw, and washer for future use.



Unscrew, lift, and remove the battery pack from the diffusion instrument; store it for future use.



Loosen the pump door screw.



Slide the pump door down; lift it to open.


---

For information about confined space entry, visit [www.indsci.com](http://www.indsci.com).



## Pump installation (continued)


---



Install a compatible extended-run-time battery in the lower receptacle of the pump case. When correctly installed, the battery's label will show.



Place the instrument in the pump case as shown.



Lower the pump door. Slide it into its fully closed, clicked-shut position.



Tighten the pump door screw.

## Pump preparation

---




Attach one end of the sample tubing to the pump inlet's nipple; attach the other end to a compatible water stop.

At each end, push on the tubing to ensure the connecting part is fully inserted into the tubing (approximately .635 cm [.25 "] ). To test for a firm connection, gently pull on the tubing.

For remote sampling applications that require the use of a probe, contact Industrial Scientific or an authorized distributor.

# Power On

To power on the instrument, press  for approximately three seconds and release it when the blue lights flash.

The instrument will complete its *self-test\**; check for these items:


- The blue and red lights flash.
- All pixels are functional on the visual test screens, which read "Industrial Scientific".
- The instrument vibrates and beeps.

Next—on the display screen—watch the *start-up sequence* for instruction, information, and access to utilities such as the zero utility. The start-up sequence will vary based on instrument settings; some of the more commonly accessible items are shown below. If the instrument has a pump installed, the start-up sequence will include a pump test; watch the display screen for instruction (see page 8).

\*If the instrument or the operator identifies a failure, contact Industrial Scientific or an authorized distributor for assistance.


## Start-up information

Assignment information




Indicates the company, person (user), and location (site) to which the instrument is assigned.

Maintenance information (dock and calibration shown)

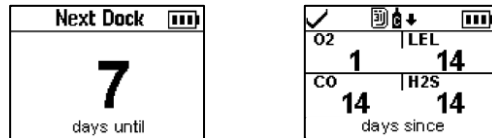

The dock information (above left) indicates the maintenance is due in the future ("days until"). The calibration information as shown here indicates when the maintenance was last performed ("days since").

Gas information (H2S shown in ppm)






Provides setpoint values (from left to right).

Top row: gas present alert, low alarm, and high alarm.

Bottom row: STEL alarm, TWA alarm, and calibration gas concentration.

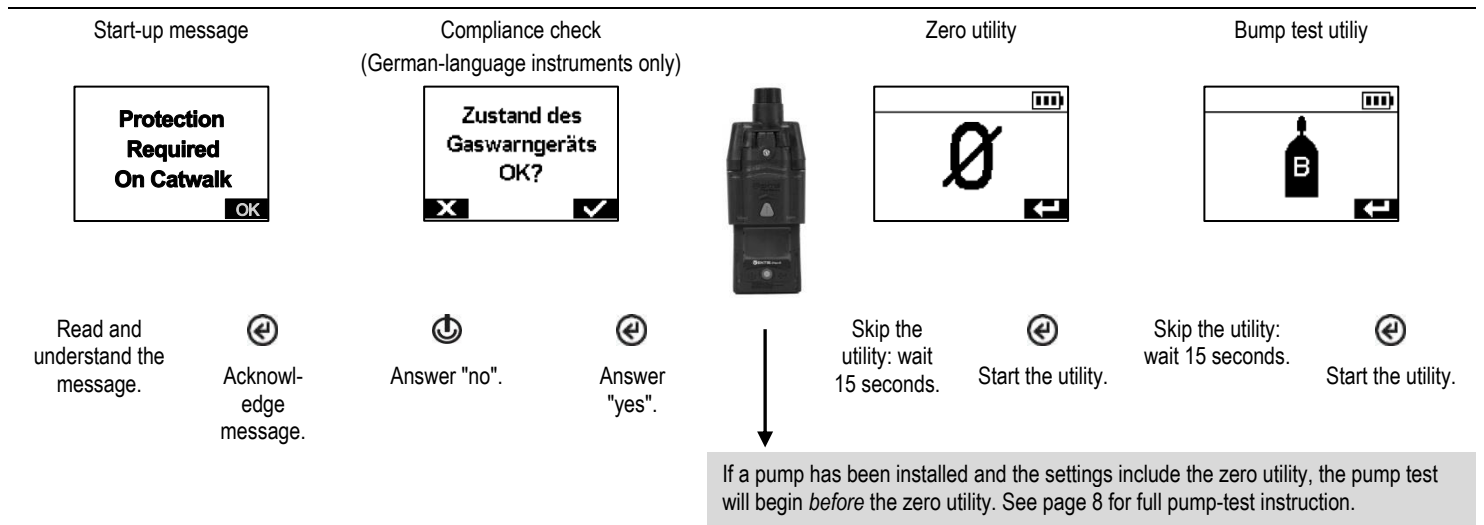
## Start-up utilities and preparation



Complete an instrument self-test any time during your workday: when the instrument is on, simultaneously press and hold  and .


# Pump test

Block inlet



When prompted, use a thumb to block the end of the sampling line.



Wait



—

While the test is in progress, the display screen will ask the instrument operator to wait. Next, the test results will be displayed as "Passed" or "Failed".

Test results: Passed




Remove thumb from the water-stop opening.  
Restart the pump: press ⚠. It may take several seconds for the pump to restart.

Test results: Failed\*



Remove thumb from the water-stop opening.



Power off the instrument.

\*A pump test failure may indicate a problem somewhere in the sampling line. Check and correct for cracks or other damage, debris, and improper installation in these areas: all sampling line connections, and the pump's inlet cap, inlet barrel, and dust filter.

# User-site Assignments

Use iAssign™ tags to change the instrument's user-site assignments. Each tag can contain a user name, site name, or both.

*Note:* An instrument's settings may not permit the use of iAssign technology.

iAssign tag



iAssign touch area



Results (confirmation and failure shown)



**Invalid Tag**

To assign the instrument to the user-site data that is on an iAssign tag, touch the tag once to the instrument's iAssign touch area.

To remove the assignment, use any one of these options:

- Touch the same tag to the instrument's iAssign touch area.
- Touch a different tag to the instrument's iAssign touch area.
- Power off the instrument.
- Dock the instrument to synchronize instrument settings with their current values in iNet, DSSAC, or Accessory Software.

Watch and listen for confirmation or failure indicators.

Confirmation

- ascending tone
- blue lights
- current user and site message

Failure

- descending tone
- red lights
- "Invalid Tag" message

If the assignment failed, it can be tried again.

For more information on assignments and iAssign technology, see the *Product Manual* at [www.indsci.com/ventispro](http://www.indsci.com/ventispro).

# Instrument Operation

Gas readings will generally look like those shown below for a five-gas instrument (enlarged for detail) and a four-gas instrument. This information screen is referred to as "Home". During operation, the instrument will display the home screen unless the user navigates to another display screen or the instrument is communicating alarm, warning, or indicator details.

## Home

The diagram illustrates the 'Home' screen for two types of gas analyzers. On the left is a five-gas instrument screen, and on the right is a four-gas instrument screen. Callouts with arrows point to specific elements on both screens.




**Five-gas instrument Home screen:**

- No fault status:** Indicated by a checkmark icon in the top left corner.
- Gas name:** Labels for O2, LEL, CO, H2S, and SO2 are positioned above their respective readings.
- Unit of measure:** Units like %vol, ppm, and LEL are shown next to the gas names.
- Current gas reading:** Large numerical values are displayed for each gas (e.g., 20.9 for O2, 0 for LEL, 0 for CO, 0.0 for H2S, 0.0 for SO2).
- Pump installed indicator:** A pump icon in the top right corner.
- Battery status (shown), temperature, and time:** A battery level icon in the top right corner.

**Four-gas instrument Home screen:**

- Temperature:** 68 F is displayed in the top right corner.
- Gas name:** Labels for O2, LEL, CO, and H2S are positioned above their respective readings.
- Unit of measure:** Units like %vol, ppm, and LEL are shown next to the gas names.
- Current gas reading:** Large numerical values are displayed for each gas (e.g., 20.9 for O2, 0 for LEL, 0 for CO, 0.0 for H2S).

To operate the instrument, press its buttons as follows:

-  View information and access utilities.
-  Start a utility or view details.
-  Turn on (or off) the instrument's high alarm.

Information and utilities that are accessible during operation will vary based on instrument settings. Some of the more commonly accessible items are shown below where instruction is provided for completing each type of utility: maintenance (bump test, zero, and calibration) and clear readings (peak, TWA, and STEL).

# Operation information

Home	Assignment information	Maintenance information (dock and calibration shown)		Gas information (shown here for H2S in ppm)	
Next display screen.	Next display screen.	Next display screen.	View span reserve percentage values.	Next display screen.	View span reserve percentage values.
Displays each sensor's current gas reading.	Indicates the company, person (user), and location (site) to which the instrument is assigned.	The dock information (above left) indicates the maintenance is due in the future ("days until"). The calibration information as shown here indicates when the maintenance was last performed ("days since"). To view optional information (span reserve percentages), press .		Provides setpoint values (from left to right). Top row: gas present alert, low alarm, and high alarm. Bottom row: STEL alarm, TWA alarm, and calibration gas concentration.	




*Span reserve percentage* is an indicator of a sensor's remaining life. When the value is less than 50%, the sensor will no longer pass calibration.

## Operation utilities

### Maintenance example

#### Bump test utility




Skip the utility: wait 15 seconds.




Start the utility.

#### Apply gas (quick bump test shown)




The sensors are set to respond to the displayed calibration gas concentrations. The instrument will wait approximately five minutes for the application of the required gas concentrations.

#### Progress



The values increase as the detected gas levels increase.

#### Results




✓ means the sensor passed.

✗ means the sensor failed.

### Clear readings example

#### Peak readings



Next display screen.



Clear the readings.

Let the gas detection experts at Industrial Scientific help you with all your learning needs.

[www.indsci.com/training](http://www.indsci.com/training)

Online and in-person training options are available.



# Alarms, Warnings, and Indicators

Alarms notify the instrument user of danger.

Warnings notify the user of a condition that needs attention.

Indicators notify the user of a status (e.g., confidence indicator).


Take seriously all alarms, warnings, and indicators, and respond according to company policy.

## Alarms

The Ventis Pro Series instruments have alarms of two intensities, high and low. When all alarm signals\* are on:

- The *high* alarm is bright red in color; it uses two different sounds and a vibration. It is fast-paced.
- The *low* alarm is similar to the high alarm, but includes blue as well as bright red light. It is medium-paced.


\*Signals (visual, audible, and vibration) vary based on instrument settings.

Alarms are persistent. They turn off when the alarm-causing event is no longer detected; however, if the instrument's alarm-latch setting is on, an alarm will remain on until the user presses  to turn it off.


Information about gas alarms is presented in different formats on the display screen as shown below for an instrument that is in high-alarm caused by the CO sensor's reading, which is now at 100 ppm.

## High alarm (gas event shown)


Instruction format\* (Evacuate shown)




Full screen alarm format\*



Readings



Event type








\*The instrument will display only one of these two formats based on the unit's settings.

Display screens shown above feature the icon (🔊) for a high-alarm gas event. When another type of event causes an alarm, the instrument's display will feature a different icon. Alarms are described below for gas and nongas events.

## Alarms (gas events)

Icon	Alarm level	Alarm event	Description
<b>OR, -OR</b>	High	Gas present (over-range)	The detected gas concentration is outside the sensor's measuring range.
🔊	High	Gas present (high-alarm)	The detected gas concentration exceeds the high-alarm setpoint.
<b>STEL</b>	High	STEL	The cumulative measure of detected gas exceeds the STEL setpoint.
🔊	Low	Gas present (low-alarm)	The detected gas concentration exceeds the low-alarm setpoint.
<b>TWA</b>	Low	TWA	The cumulative measure of detected gas exceeds the TWA setpoint.

## Alarms (nongas events)

Icon	Alarm level	Alarm event	Description
	High	Man down	The instrument has not moved for the set period of time. To turn off the alarm, press and hold  .
	High	Panic	The user has pressed the instrument's panic button and held it long enough to turn on the panic alarm. To turn off the alarm, press and hold  .
<b>PUMP FAULT</b>	High	Pump fault	The pump is not operational. A pump fault may indicate a problem somewhere in the sampling line.
<b>ERROR 408</b>	High	System	The instrument is in failure (error code 408 shown here) and is not operational.
	High	Critical low battery	The instrument has shut down and is not operational.

## Warnings








Warnings turn on and off repeatedly. The more urgent the warning, the shorter the time between on-off occurrences: a warning that repeats every two seconds is more urgent than a warning that repeats every thirty seconds. Warnings persist until the issue is resolved.

When all signals\* are on, a warning appears as a short burst of red and blue light mixed with sound and vibration.

Warning events are defined below, followed by their display screen reproductions.

\*Signals (visual, audible, and vibration) vary based on instrument settings.

## Warnings


Icon	Warning frequency	Warning event	Description
	Every 2 seconds	Man down	The instrument has not moved for the set period of time. To turn off the warning, move the instrument.
	Every 8 seconds	Gas alert	A detected gas concentration may be approaching alarm levels. To turn off the warning, press and hold  .
	Every 10 seconds	LEL-Low O <sub>2</sub>	LEL and O <sub>2</sub> sensors are installed and the concentration of O <sub>2</sub> is insufficient for LEL sensor functionality.
	Every 15 seconds	Sensor failure	If the sensor has failed a procedure, this icon will alternate with text that indicates what failed ( <b>CAL</b> , <b>BUMP</b> , or <b>Ø</b> ).
	Every 30 seconds	Instrument maintenance overdue (bump test shown)	The instrument is in need of some form of maintenance.
	Every 60 seconds	Low battery	The instrument's battery is low.

### Sample warning display screens


Man-down warning (120-second pre-alarm countdown shown)



Gas alert (H<sub>2</sub>S shown)




Instrument issue (LEL sensor failure shown)



Maintenance overdue (bump test for CO and H<sub>2</sub>S shown)



Low battery



## Indicators


Most indicators turn on once, then off; only the confidence indicator persists, repeating every 90 seconds. If all signal\* settings are on, status indicators will look and sound like this:

Indicator	Status	Color	Sound
User or site assignment, calibration, or bump test	Confirmation	Blue	Ascending
User or site assignment, calibration, or bump test	Failure	Red	Descending
Confidence indicator	Instrument on	Blue	Beep

\*Signals (visual, audible, and vibration) vary based on instrument settings.


## Power Off

Countdown




Hold for the full five-second countdown.

Enter security code\*





Enter the displayed value.

Change the displayed value.



Quick Status

Check available battery power, installed sensors, and serial number any time the instrument is off: simultaneously press and hold  and .

\*Activation of this display screen and the security code value vary based on instrument settings





The company **Industrial Scientific Corporation**, Pittsburgh, Pennsylvania USA, declares that the following new material intended for use in Explosive Atmospheres:  
*(La société Industrial Scientific Corporation, Pittsburgh, Pennsylvania USA, atteste que le matériel neuf destiné à être utilisé en Atmosphères Explosives désigné ci-dessus.)*

**Gas detector (Détecteur de gaz) VENTIS PRO 4/5**  
comply with the requirements of the following European Directives:  
*(est conforme aux exigences des Directives Européennes suivantes.)*

**I) The European Directive ATEX 94/9/EC of 23/03/94: Explosive Atmospheres**  
*Directive Européenne ATEX 94/9/EC du 23/03/94: Atmosphères Explosives*

**No. of EC type examination certificate:**

*(N° d'attribution CE de Type du matériel.)*  
Issued by the Notified Body no. 0539:  
*(Délivré par l'Organisme notifié sous le numéro 0539)*


**DEMKO 15 ATEX 1571**

UI, International DEMKO AS, LYSKEAR 8  
P.O. Box 514, DK - 2730, HERLEV, DENMARK

**Reference European Standards (Normes européennes de référence):**

Rules of construction (Règles de construction): EN 60079-0:2012+A1:2013, EN 60079-1:2007  
EN 60079-11:2012

**Category (Catégorie):**

 II G / I M1  
II 2G / I M1 with IR sensor  
Ex ia I/IC T4 Ma Ga  
Ex d ia I/IC T4 Ma Gb with IR sensor  
Tamb -40°C to +50°C IP64  
Tamb -20°C to +50°C with IR sensor

**Production Quality Assurance Notification No. of the Pittsburgh factory (SIRA 00 ATEX M0080)**  
*(N° de la Notification Assurance Qualité de Production de l'usine de Pittsburgh)*

Issued by the Notified Body no. 0518:  
*(Délivré par l'Organisme notifié sous le numéro 0518)*

SIRA Certification Services, Rake Lane  
Eccleston, Chester CH4 9JN, UK

**II) The European Directive EMC 2004/108/EC of 15/12/04: Electromagnetic Compatibility**  
*Directive Européenne EMC 2004/108/EC du 15/12/04: Compatibilité Electromagnétique*

**Harmonised applied standards:** EN 50720:2015, EN 501 489-1 V1.8.1:2008-04, EN 501 489-17  
*(Normes harmonisées applicables)* V2.2.1:2012-09

**III) The European Directive R&TTE 1999/5/EC of 9/03/99: Radio & Telecommunications Terminal Equipment**  
*Directive Européenne R&TTE 1999/5/EC du 9/03/99: Equipements radio et équipements terminaux de télécommunication*  
**Harmonised applied standards:** EN 300 330-1 V1.8.0:2014-06, EN 300 328  
*(Normes harmonisées applicables)* V1.8.1:2012-06

**On behalf of the manufacturer**

*Pour le fabricant*

**Industrial Scientific Corporation**

3 Rue de la République  
Pittsburgh, PA 15205 USA  
Tel: +01 412 788 4353  
www.indsci.com

**On behalf of the manufacturer representative in EC**

*Pour le représentant du fabricant dans l'UE*

**Industrial Scientific France SAS**

5 Rue de la République  
Pittsburgh, PA 15205 USA  
Tel: +33 (0)1 5732 92 61

**The ATEX Authorized Representative**

*Le Représentateur Autorisé ATEX*

  
**Tom Milkulin**

Global Director, Product Development  
*(Directeur Technique)*  
15 January 2016

**OUR MISSION**

Preserving human life on, above and below the earth.  
Delivering highest quality, best customer service ...  
every transaction, every time.



***INDUSTRIAL***  
***SCIENTIFIC***

---